


CORRECTION

Open Access



Correction: Value assessment of artificial intelligence in medical imaging: a scoping review

Iben Fasterholdt^{1*} , Mohammad Naghavi-Behzad^{2,3}, Benjamin S. B. Rasmussen^{2,4,6}, Tue Kjølhed¹, Mette Maria Skjøth⁵, Malene Grubbe Hildebrandt^{1,2,3} and Kristian Kidholm¹

Correction: BMC Medical Imaging (2022) 22:187
<https://doi.org/10.1186/s12880-022-00918-y>

Following the publication of the original article [1], it was brought to our attention that an error had been introduced during typesetting:

The incorrect word “screnned” was inadvertently inserted under “1598 duplicates removed” in Fig. 1.

The incorrect word has now been deleted and the correct Fig. 1 is included in this Correction.

The original article has been updated.

Published online: 23 January 2023

Reference

1. Fasterholdt, et al. Value assessment of artificial intelligence in medical imaging: a scoping review. *BMC Med Imaging*. 2022;22:187. <https://doi.org/10.1186/s12880-022-00918-y>.

Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

The original article can be found online at <https://doi.org/10.1186/s12880-022-00918-y>.

*Correspondence:

Iben Fasterholdt
if@rsyd.dk

¹ CIMT – Centre for Innovative Medical Technology, Odense University Hospital, Sdr. Boulevard 29, Entrance 102, 4rd Floor, 5000 Odense C, Denmark

² Department of Clinical Research, University of Southern Denmark, Odense, Denmark

³ Department of Nuclear Medicine, Odense University Hospital, Odense, Denmark

⁴ Department of Radiology, Odense University Hospital, Odense, Denmark

⁵ Department of Dermatology and Allergy Centre, Odense University Hospital, Odense, Denmark

⁶ CAI-X – Centre for Clinical Artificial Intelligence, Odense University Hospital, Odense, Denmark



© The Author(s) 2023. **Open Access** This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>. The Creative Commons Public Domain Dedication waiver (<http://creativecommons.org/publicdomain/zero/1.0/>) applies to the data made available in this article, unless otherwise stated in a credit line to the data.

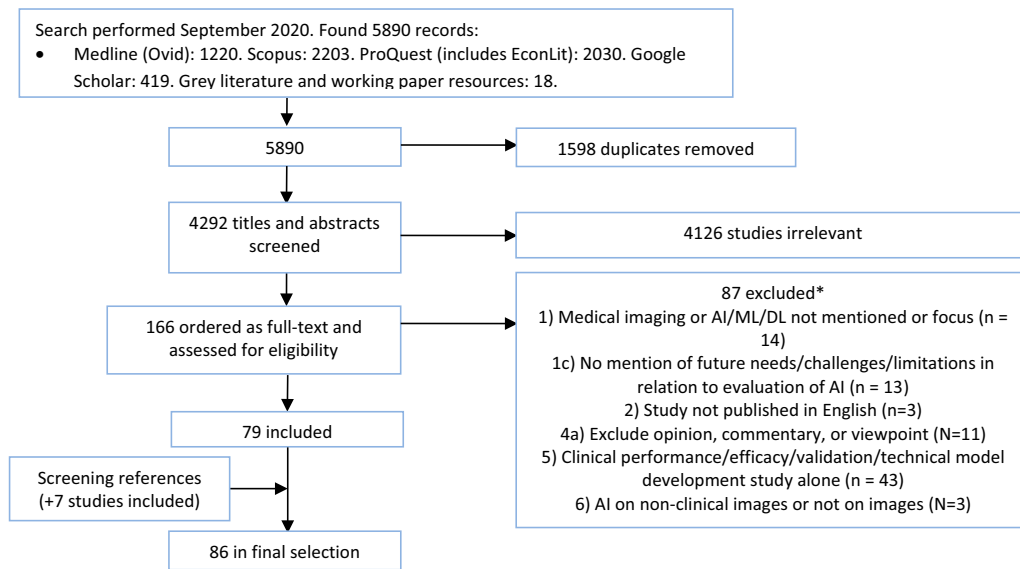


Fig. 1 PRISMA flow chart for selection of the studies. *The number in front of the list with exclusion reasons refers to the exclusion criteria in Table 2